


Isis Height Adjustable Bath Pre installation requirements

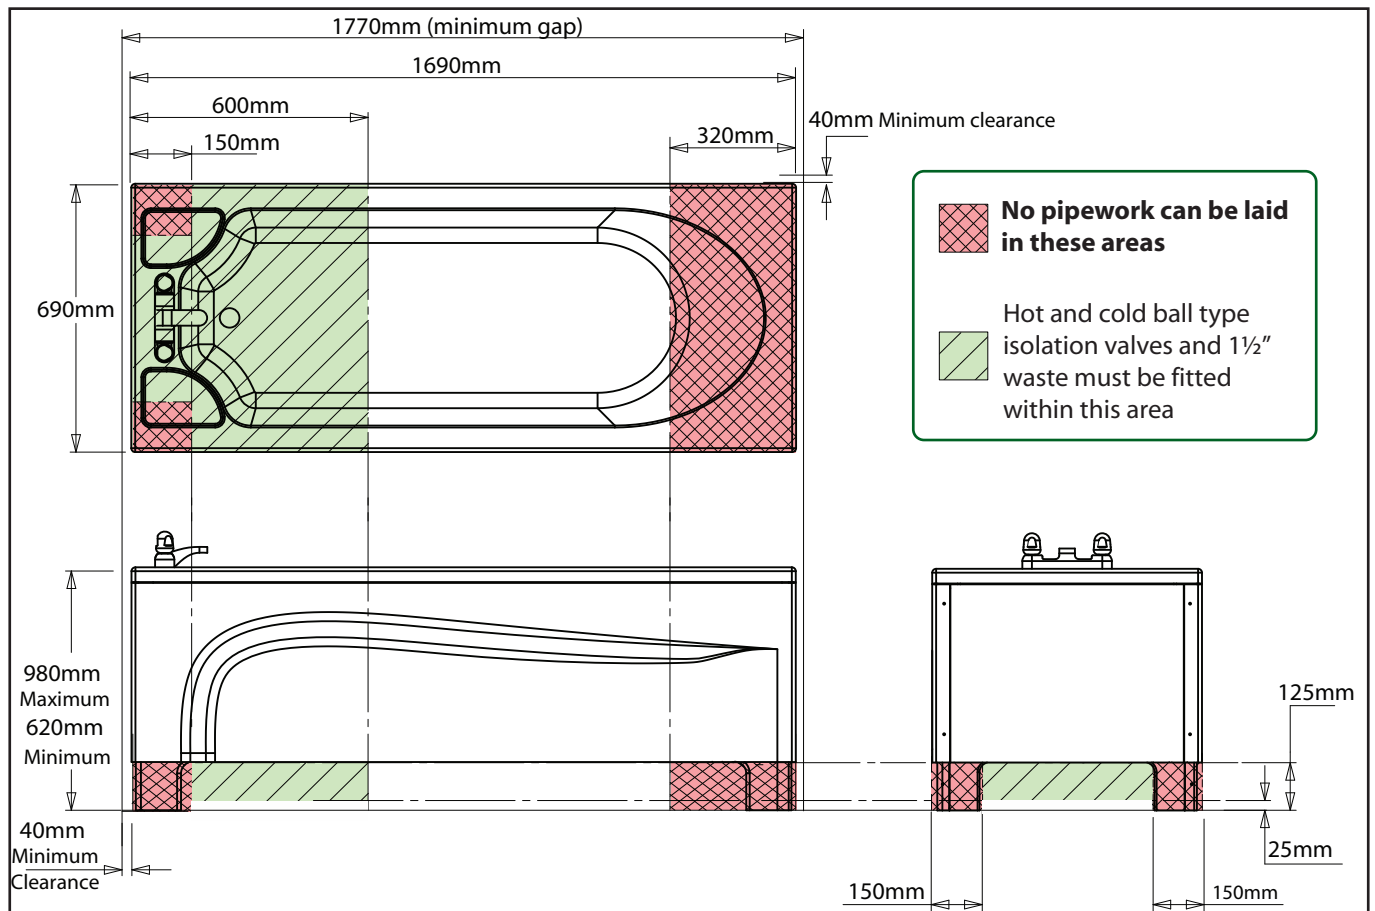

Plumbing

Hot and cold ball type isolation valves (22mm) must be mounted entirely within the green hatched areas shown above, maximum height above the floor 150mm.
The 1½" waste also needs to be fitted entirely within the green hatched area shown above - maximum height of 150mm from the floor. No pipework can be laid in the areas hatched red.

Thermostatic Taps require a minimum water pressure of 1 bar (14.5psi) and a maximum of 10 bar. The pressure ratio between hot and cold must not exceed 5:1.

Electrics

230 volt, 13 amp waterproof flex outlet, located within 3 metres of the bath, supplied by a 30mA RCD protected fused spur is required.

Fixing

The Isis bath is floor standing and secured to the floor. Floors must have sufficient depth in order to receive 30mm long screws and associated wall plugs (please indicate any under-floor heating so that alternative arrangements can be made). Walls need to be plumb, smooth and clear of obstructions from floor level to 1050mm. Skirting boards may be left in place and the wall may be tiled.

Isis Height Adjustable Bath Pre installation checksheet



Please read and check the sections below before ticking each box

Plumbing

1. Hot and cold supplies are installed in the green shaded areas shown overleaf terminating in 22mm ball type isolation valves fitted up to a maximum height of 150mm from the floor

2. 1½" waste is installed in the green shaded areas shown overleaf up to a maximum height of 150mm from the floor

Electrics

A 230 Volt 13 Amp waterproof flex outlet, located within 3 metres of the bath, supplied from a 30mA RCD protected fused spur has been supplied and is connected
Please identify location.....

2. We are willing to have the Astor-Bannerman installer run flex encased in surface conduit from the site of the outlet to the bath

Floor

1. The floor is finished, free of obstructions around legs and suitable for 30mm long screws

2. The floor is of concrete/wooden construction (delete as appropriate)

3. Is there under-floor heating in the area of proposed installation? YES NO
IF YES PLEASE CONTACT ASTOR BANNERMAN

Walls

1. Walls are plumb, smooth and clear of obstructions from floor level to 1050mm from the floor

Access

1. The unit is not required to be installed upstairs/through difficult access
Or

2. The unit is required to be installed upstairs/through difficult access but necessary arrangements have been made to assist the Astor-Bannerman engineer

3. The bath will be used as part of A: single user environment B: a multi user environment

Important

We confirm that 230 Volt mains power supply (not temporary supply), hot and cold water supplies and waste pipe will be connected and operational BEFORE the Astor-Bannerman engineer visits.

This last box must be ticked before we are able to release the goods for installation

We understand that any waiting time will be charged to us and should the site require a second visit due to the above requirements not being met an additional £350.00 per visit will be charged and we agree to pay those charges

Signed Date
Print name Job number
Site address

Astor Bannerman (Medical) Ltd. Fax: 01242 821110
Unit 11f Coln Park Email:sales@astorbannerman.co.uk
Andoversford Web:www.astorbannerman.co.uk
Gloucestershire GL54 4HJ Tel.: 01242 820820