

Beka Heela Height-Adjustable Bath PRE INSTALLATION REQUIREMENTS

Astor-Bannerman requires one of the following three installation options to be chosen and in-situ before the installation engineer arrives on site.

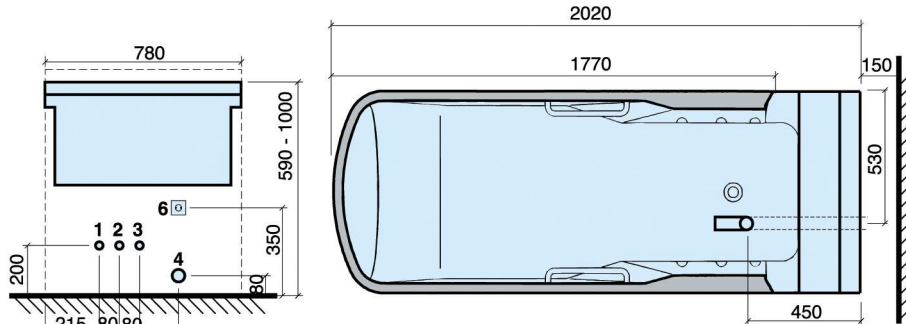


Figure A - wall connection - direct

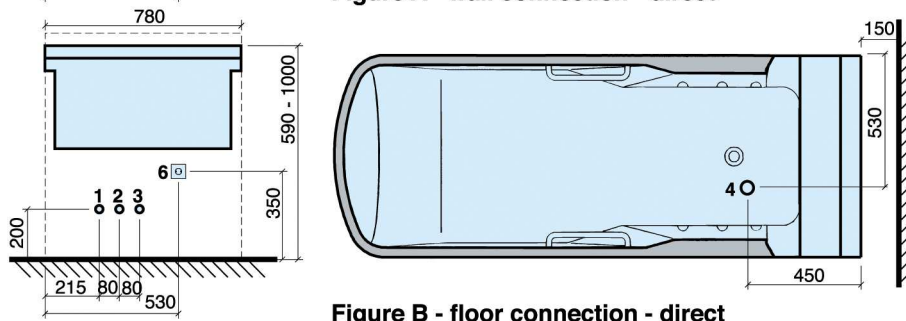


Figure B - floor connection - direct

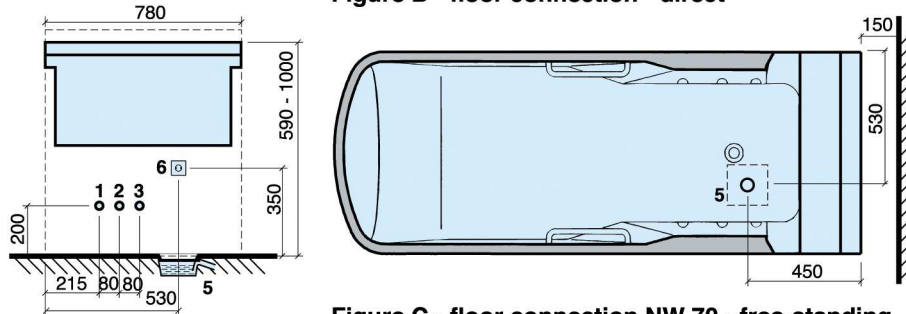


Figure C - floor connection NW 70 - free-standing

Diagram key

1. 3/4" BSP male hot water inlet valve
2. 3/4" BSP male cold water inlet valve
3. 1/2" male central disinfection connection (if applicable)
4. ø50mm household waste pipe, 80mm above floor surface
5. Gulley trap (capacity 3.5 l/sec)
6. Electrical connections: 230v/50Hz, 1.5mm², 1.25kW, flex length 1.5m

All dimensions are provided in millimetres

Astor-Bannerman (Medical) Ltd
 Unit 11f Coln Park
 Andoversford
 Cheltenham
 Gloucestershire, GL54 4HJ
Tel: 01242 820820 **Fax:** 01242 821110

**BEKA HEELA HEIGHT-ADJUSTABLE BATH
PRE INSTALLATION REQUIREMENTS CHECKSHEET**
This sheet must be completed and returned before installation can take place

Please tick to confirm:

WALL

1. Walls are free of obstructions 0-1000 mm from the floor

FLOOR

1. Floor is free of obstructions around the base
2. Floor is of concrete/wooden construction (delete as appropriate)

PLUMBING

1. Hot and cold supplies are installed in shaded areas shown overleaf terminating in ¾" BSP washing machine check valves (please mark positions overleaf) up to a max. height of 200mm from the floor
2. ø50mm household waste pipe is installed up to a max. height of 80mm from the floor surface

ELECTRICS

1. Waterproof fused spur is provided within 3 metres of the bath
PLEASE IDENTIFY LOCATION

ACCESS

One of the following options **MUST** be chosen.

1. The unit is not required to be installed upstairs
or
2. The unit is required to be installed upstairs

IMPORTANT

We confirm that a 240 volt power supply for the unit (not temporary supply), hot and cold water and waste pipes will be connected and operational **BEFORE** the Astor-Bannerman engineer visits. We have made sure that access for the engineer will not be a problem.

We understand that any waiting time will be charged to us and should the site require a second visit due to the above requirements not being met an additional £350.00 per visit will be charged and we agree to pay those charges.

Please note: Following installation, 240 volt supply must be left **ON** to the bath for constant charging of the batteries.

Signed Date

Print name Job number

Site address