


Interbath Height Adjustable Bath Pre installation requirements

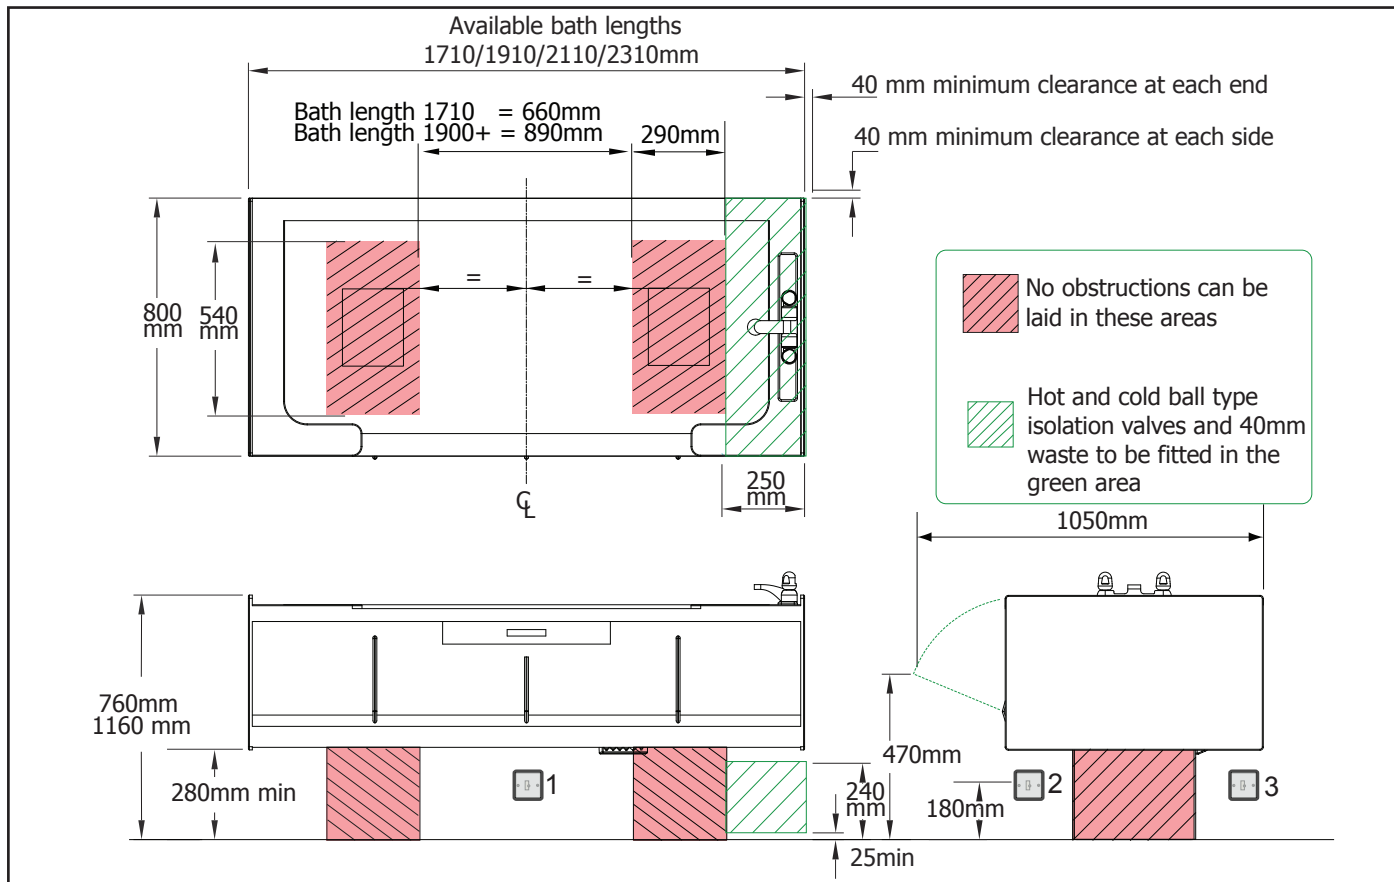

All wall and floor decoration must be complete prior to installation.

NOTE: Floors must be flat and level in the area where the bath is to be installed.
If this is not possible Astor Bannerman MUST be informed prior to installation.

Plumbing

We require Hot and cold ball type isolation valves (22mm) fixed entirely within the green area shown above. A 40mm waste is required within the green area no more than 80mm from the floor. Occasionally a twin waste system is specified, contact Astor Bannerman for details.

Thermostatic Taps require a minimum dynamic water pressure of 1 bar (14.5psi) and a maximum of 10 bar. The pressure ratio between hot and cold must not exceed 5:1.

NOTE: These taps are not compatible with NON-Modulating Combination Boilers.

Electrics

We require a 230 volt, 1.25kW waterproof flex outlet, located within the footprint of the bath at any of the wall positions (1,2,3), supplied by a protected fused spur.

Fixing and Positioning

The Interbath is floor standing and secured to the floor. Floors must flat and level with sufficient depth to accept 50mm long M8 expansion bolts (please indicate any under-floor heating so that alternative arrangements can be made).

Walls need to be plumb, flat and clear of obstructions from floor level to 1200mm. Allow a minimum gap of 40mm at each end and the fixed side plus a 900mm minimum clearance for the hinged door side.

If a Neatfold stretcher is specified, extra clearance may be required. Contact Astor Bannerman for details.

Floors must be strong enough to support the weight of the bath.

Skirting boards may be left in place. The wall and floor decoration must be COMPLETE prior to installation.

Astor Bannerman (Medical) Ltd. Fax: 01242 821110

Unit 11f Coln Park Email:sales@astorbannerman.co.uk

Andoversford Web:www.astorbannerman.co.uk

Gloucestershire GL54 4HJ Tel.: 01242 820820

Form 09O V08 121211

Interbath Height Adjustable Bath Pre installation checksheet



Please read and check the sections below before ticking each box

THIS SHEET MUST BE COMPLETED AND RETURNED BEFORE INSTALLATION CAN TAKE PLACE

Plumbing

1. Hot and cold supplies are installed in the green shaded area shown overleaf terminating in 22mm ball type isolation valves fitted at a max. height of 240mm from the floor.

2. A 40mm waste is installed in the shaded area shown overleaf and is within 80mm from the floor.

Electrics

1. A 230 Volt 1.25kW waterproof flex outlet, located as shown overleaf, supplied from protected fused spur is installed and operational.
Please identify location.....

2. We are willing to have the Astor-Bannerman installer run flex encased in surface conduit from the site of the flex outlet to the bath.

Floor

1. The floor is finished, free of obstructions around the base area.

Walls

1. Walls are plumb, flat and clear of obstructions from floor level to 1200mm from the floor.

2. There is sufficient space around the bath to provide a minimum 40mm gap at the fixed side and each end plus 900mm on the hinged door side.

Access

1. The unit is not required to be installed upstairs/through difficult access.
Or

2. The unit is required to be installed upstairs/through difficult access but necessary arrangements have been made to assist the Astor-Bannerman engineer.

3. The bath will be used as part of A: single user environment B: a multi user environment

Important

We confirm that 230 Volt mains power supply (not temporary supply), hot and cold water supplies and waste pipe will be connected and operational BEFORE the Astor-Bannerman engineer visits.

This last box must be ticked before we are able to release the goods for installation

We understand that any waiting time will be charged to us and should the site require a second visit due to the above requirements not being met an additional £845.00 per visit will be charged and we agree to pay those charges.

Signed Date
Print name Job number
Site address