




Avero Height Adjustable Bath Pre Installation Requirements

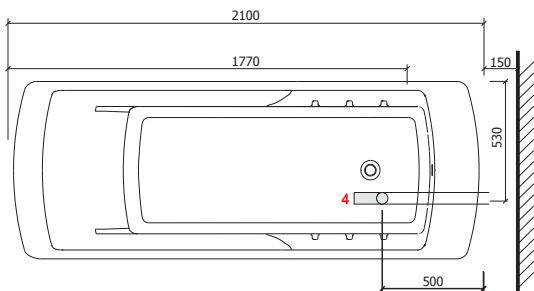

Option A-Wall drain connection

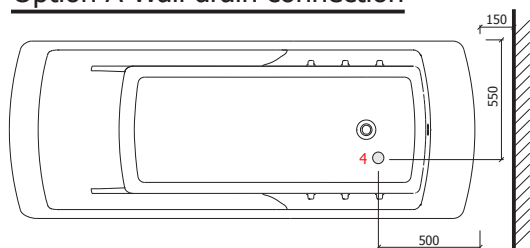

Option B-Floor drain connection

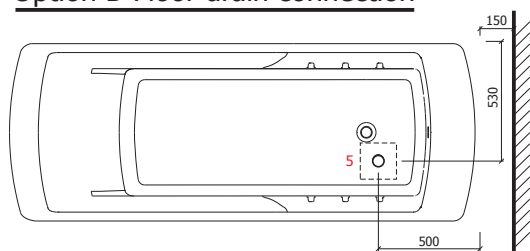

Option C-Floor Gully connection

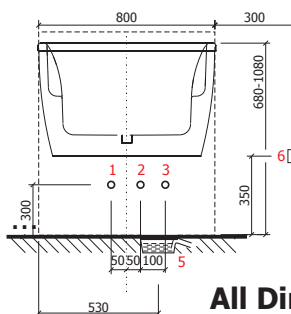




Diagram key

1. 22mm ball type isolator valve hot.
2. 22mm ball type isolator valve cold.
3. 1/2" male connection for central disinfection system; (if applicable)
4. 1 1/2" waste pipe; maximum 80mm above floor.
5. Gully trap; (capacity 3.5 l/sec)
6. Electrical connections:
Waterproof ,RCD protected, fused spur
230v/50Hz. 1.25kW.

All Dimensions in millimeters

Plumbing

Hot and cold ball type isolation valves (22mm) need to be supplied; maximum height of 300mm from the floor. The 1 1/2" waste also needs to be supplied in one of the above options; maximum height of 80mm from the floor. All Pipework must be supplied in **one** of the options shown above and indicated overleaf.

Thermostatic taps require a minimum water pressure of 1 bar (14.5psi) and maximum of 10 bar (145psi).

Maximum pressure ratio; cold : hot must not exceed 5:1

Electrics

We require a 240 volt, 1.25kW **waterproof** mains outlet, supplied from a 30mA RCD protected fused spur located as in one of the options shown above.

Fixing

The Avero bath is floor standing. Please indicate any under-floor heating. (In case a Floor Mounted Shower Gantry is required).

Walls need to be plumb, smooth and clear of obstructions from floor level to 1080mm.

Skirting boards may be left in place and the wall tiling is to be complete prior to installation.

Avero Height Adjustable Bath Pre Installation Checksheet



This sheet must be completed and returned before installation can take place

Please read and check the sections below carefully before ticking each box



Plumbing

- Hot and cold supplies are installed in one of the options shown overleaf terminating in 22mm ball type isolation valves up to a max. height of 300mm from the floor.
- 1½" waste is installed in shaded areas shown in the options overleaf up to a maximum height of 80mm above the floor. Enter Option Chosen (A,B,C).....

Electrics

- A 240 volt, 1.25kW **waterproof** mains outlet, supplied from a 30mA RCD protected fused spur, located as in one of the options shown overleaf is installed.
- We are willing to have the Astor-Bannerman installer fit flex encased in surface conduit from the site of the outlet (in point 1 above) to the bath.

Floor

- The floor is finished, free of obstructions around the base and suitable for 30mm screws.
 - The floor is of concrete/wooden construction (delete as appropriate).
 - Is there under-floor heating in the area of proposed installation? Yes No
- If Yes Please contact Astor Bannerman.

Wall

- Walls are plumb, smooth and clear of obstructions from floor level to a height of 1080mm. Skirting boards may be left in place and the wall tiling is to be complete prior to installation.

Access

- The unit is not required to be installed upstairs/through difficult access.
- The unit is required to be installed upstairs/through difficult access but necessary arrangements have been made to assist the Astor-Bannerman engineer.
- The bath will be used as part of a single user environment. multi user environment.

IMPORTANT

We confirm that 240 volt mains power supply (not temporary supply), hot and cold water supplies and waste pipe will be connected and operational BEFORE the Astor-Bannerman engineer visits.

This last box must be ticked before we are able to release the goods for installation. We understand that any waiting time will be charged to us and should the site require a second visit, due to the above requirements not being met, an additional £350.00 per visit will be charged and we agree to pay those charges.

Signed..... Date.....

Print name..... Job number.....

Site address

.....